



OPERATION MANUAL

NR Recorder

CE

2797

Copyright © Norav,

No part of this publication may be reproduced in any material form (including photocopying or storing it in any medium by electronic means whether or not transiently or incidentally to some other use of this publication) without the prior written permission of the copyright owner, or under the terms of a license issued by the copyright owner.

The information contained in this document is subject to change without notice. Norav is neither responsible for nor liable to anyone in connection with this document.



Manufactured by:

Norav Medical GmbH

Christof-Ruthof-Weg 10

55252 Mainz-Kastel

Germany

Telephone: +49 (0) 6134-567983-0

Faximile: +49 (0) 6134-567983-01

E-Mail: info@norav.com

The NR digital Recorder conforms to MDD 93/42/EEC .



Caution

Federal Law restricts this device to sale by or on the order of a licensed physician or healthcare provider

Disclaimer

This system is intended as a decision support system for persons who have received appropriate medical training, and should not be used as a sole basis for making clinical decisions pertaining to patient diagnosis, care, or management. Any application of medical information from the program, other than the original design or intended use thereof, is not advised and considered a misuse of the software product.

Norav Limited Warranty

Norav products are warranted to be free from manufacturing and material defects for a period of one (1) year from the date of shipment from Norav or the dealer to the original purchaser.

Excluded from this warranty are expendable supply items including, but not limited to, electrodes, lead wires, patient cables, and batteries. This warranty does not apply to any product that Norav determines that it has been modified or damaged by the customer.

Except for the express warranties stated above, Norav disclaims all warranties including implied warranties of merchantability and fitness. The stated express warranties are in lieu of all obligations or liabilities on the part of Norav for damages, including but not limited to, special, indirect, or consequential, arising out of or in connection with the use or performance of Norav products.

Any action for breach of warranty shall be commenced within one (1) year of said breach or be forever barred. Any repairs made to the product that are not covered by the warranty shall be billed to the customer.

For service or technical support contact your local supplier or Norav Medical.

Contents

Disclaimer	3
Norav Limited Warranty	3
Symbols used in this manual:	6
Device label symbols:.....	7
Description	8
Recorder Feature Matrix.....	8
Intended use.....	8
Contraindications and adverse effects	9
Warning and Precautions.....	9
Controls and Indicators.....	12
Memory Card (SD card).....	13
Main Battery	14
Insert Battery	14
RTC Back up Battery	14
Electrode Application.....	15
Attaching the electrodes	15
Electrode Placement	16
Patient Cable Connection	17
Connecting:	17
Disconnecting:.....	17
Screen Navigation	18
Common Workflow.....	21
Holter mode (for NR-302/314/1207/1207-3 models).....	21
Holter+ mode (for 1207-3 model only)	21
ECG mode (for NR-314-T/1207-E/1207-3 models).....	21
ECG+ mode (for 1207-3 model only)	21
ECG Recording Detailed Instructions	22
Starting New test	22
1. Prepare Recorder	22
2. Enter Patient Information (for Holter, Holter+ and ECG+ mode).....	22
3. Check ECG Leads	22
4. Start Recording (for Holter, Holter+ and ECG+ mode)	22
Acquire ECG On-line (for Holter+, ECG and ECG+ mode).....	22
Enter a Diary Event (for Holter, Holter+ mode).....	23
Add a New Patient Marker (for ECG+ mode only).....	23
Stop/Pause/Restart the ECG Recording (for ECG+ mode only)	23
To Stop Holter Recording (for Holter and Holter+ mode)	23
Data Download	23
Maintenance and Cleaning	25
Storage.....	27
Service	27
Calibration.....	27
Troubleshooting.....	28
Technical Specifications.....	29
ECG Cables and Accessories	30
Electromagnetic Emissions and Immunity Information	31
FCC information.....	33
Document History	34

Symbols used in this manual:




WARNING

Warnings call attention to possible hazards involving potential damage or injury to persons.



Caution

Cautions refer to practices necessary to protect against potential damage or loss to equipment. Pay careful attention to instructions.



Note

Notes provide pertinent information to help obtain optimum performance from the software or signify an important step or procedure that requires special attention.

Device label symbols:

Symbol	Description
	Applied part type BF
	Defibrillator-proof type CF applied part
	Defibrillation protection in patient cable
	Caution
	Refer to operation manual NOTE On ME EQUIPMENT "Follow instructions for use"
	The recorder is not suitable for measurements conducted on children weighing less than 10 kg (formation of loops in the patient cable!).
	IP protection class
	Device Serial Number
	Device Reference Number
	Date of manufacture
	Use AA (R6) batteries.
	Contains FCC certified Bluetooth module
	Disposal of the device in accordance with the EU Directive 2002/96/EC (WEEE).
	Indicates the proper orientation of battery to be installed
	By prescription only. U.S. Federal Law restricts this device to sale on order of a physician only.
	Contains MIC certified Bluetooth module
	Contains RCM certified Bluetooth module

Description

The NR device is a digital ECG recorder which allowing continuous recording of ECG waveforms in daily life. This instrument features digital recording of ECG waveforms on the SD Flash memory card. The NR can also store information of pacemaker pulses, acceleration sensor, respiration signal and voice recording. The NR-1207-x Models can utilize a 10-lead electrode hookup and placement to provide 12 channels of full disclosure for analysis.

The NR is a part of a conventional ambulatory ECG system where the data is recorded on a memory card that may be removed from the device after the recording is complete. The memory card is then placed in a card reader that is connected to the Computer Analysis System. Optionally the NR can be directly connected to the Computer Analysis System via special USB cable.

By following the instructions provided by Computer Analysis System, the recorded ECG data is downloaded from the memory card and analysis.

ECG data and patient data can be transmitted via a Bluetooth connection (BT module from Bluegiga) from NR to the Computer Analysis System and also from Computer Analysis System to the NR.

The NR shall connect only to computers that are complied with EN60950-1 and have an operating system of Windows 7 or newer.

Recorder Feature Matrix

The following table is showing the available features depending on the recorder variant.

	ECG channels	Patient cable Leads	Pacemaker detection	Acceleration sensor	Respiration signal	Voice recording	Bluetooth communication	USB communication	Ambulatory (Holter recording)	Resting ECG	Stress ECG	Telemetry ECG
NR-302	3	3,5,7	yes	no	no	no	no	yes	yes	no	no	no
NR-314	3	3,5,7	yes	yes	yes	yes	yes	yes	yes	no	no	no
NR-314-T	6	4,5	yes	no	no	no	yes	no	no	no	no	yes
NR-1207	3,12	3,5,7,10	yes	yes	yes	yes	yes	yes	yes	no	no	no
NR-1207-3	3,6,12	3,4,5,7,10	yes	yes	yes	yes	yes	yes	yes	yes	yes	yes
NR-1207-E	6,12	4,5,10	yes	no	no	no	yes	no	no	yes	yes	no

Intended use

The NR recorder is a multi-model product which used for acquiring, recording (to SD card), transmitting (via BT), analyzing (using software), displaying and printing (using software) ECG's.

Intended for patients requiring:

- Ambulatory (Holter) recording
- Use within the physician office setting by the medical professional
 - Resting ECG (using Bluetooth communication)
 - Stress ECG (using Bluetooth communication)
 - Telemetry ECG (using Bluetooth communication)

Such device is most frequently used for the indications below:

- Evaluation of symptoms suggesting arrhythmia or myocardial ischemia
- Evaluation of ECG documenting therapeutic interventions in individual patients or groups of patients
- Evaluation of patients for ST segment changes
- Evaluation of a patient's response after resuming occupational or recreational activities (For example, after myocardial infarction or cardiac surgery)
- Clinical and epidemiological research studies
- Evaluation of patients with pacemakers
- Reporting of QT interval

Contraindications and adverse effects

There are no known contraindications or adverse effects for using Holter equipment.

Warning and Precautions



WARNING

- The NR recorder (NR-314-T, NR-1207-E, NR-1207-3) is protected against the defibrillator, when a defibrillation protected patient cable is used. (see table: “ECG Cables and Accessories” with part numbers).
To avoid the possibility of injury/hazardous situations during cardiac defibrillator use, a protected against the defibrillator cables must be used.
To avoid the possibility of injury during patient defibrillation, do not come into contact with device or patient cables. Additionally, proper placement of defibrillator paddles in relation to the electrodes is required to minimize harm to the patient.
- The NR recorder (NR-314, NR-302, NR-1207) is NOT protected against the defibrillator. When using the defibrillator, remove NR recorder from the patients.
- The NR recorder is not intended for use on infants weighing less than 10 kilograms (22 pounds).
- The NR recorder is not protected against the high-frequency surgical apparatus. When using the high-frequency surgical apparatus, remove NR recorder from the patient.
- NR recorder is not directly applicable to the heart.
- Do not use the NR recorder in an area where using combustible or flammable gas or liquid such as anesthetic, oxygen, or hydrogen.
- The NR's power supply and patient circuit are not distinctly isolated. Only use batteries that are specified for the operation of this recorder. Do not, under any circumstances, use a power supply unit - this could threaten the patient's life.
- Any attempt to use NR recorder in an area where MRI is operating will mutually generate negative effects.
- Make sure that the electrode plug (patient side) never comes into contact with live parts. Do not operate the recorder near exposed live parts.
- Store the NR recorder safely away from children.
- Before each recording and before attaching sensors or electrodes to the patient, check the casing and the ECG patient cable for damage which may have occurred, for example, due to mechanical overload, falling from a great height or wear and tear (chafed patches on the cable). Do not use the instrument or the cable if you detect cracks, melted areas or any other signs of damage to the cable or housing.

**Caution**

- Store the NR recorder in an area free from water or humidity
- Take care to avoid areas subject to high humidity, poor ventilation and direct sunlight; store the NR recorder in an area free from any adverse effects of surrounding air containing dust, sodium, and sulfur.
- Do not store the NR recorder in an area where chemicals are kept, or which is exposed to chemical fumes or vapors.
- Do not connect NR recorder other than the specified equipment for your safety and optimal performance.
- Never attempt to modify or to disassemble the NR recorder.
- Do not open the case except for by our service person.
- Check that electrodes are correctly and completely installed.
- When using NR recorder in combination with any other equipment, refer to a qualified service technician for correct handling.



**Caution**

- When changing the batteries, make sure you insert them correctly (polarity). The polarity is indicated in the battery compartment.
- Do not leave the batteries in the NR recorder when it is not in use. Damage to the recorder could result from corrosion of the batteries.
- Even though that the NR recorder is protected against ingress of liquids (IP22), during a recording prevent it from being exposed to liquids. The recorder is not suitable for use in the bath tub or shower.
- During recording, make sure that the cable lead wires are not caught by the moving parts of a machine or sport equipment. This could lead to damage or injury (e.g. if loops are formed in the cable lead wires).
- Take care to prevent chemicals/liquids from entering the connectors or internal part of the recorder.
- Any attempt to use cleaner containing organic solvent, thinner, toluene, or benzene for cleaning of the NR recorder will generate the damage of the housing.
- When cleaning NR recorder, wipe with a cloth soaked with regular household cleaner diluted with water.
- Do not polish the housing with abrasive or chemical cleanser.
- Do not, under any circumstances, insert objects in the ECG Connector slot, SD card slot or the battery compartment other than NR ECG Cable connector, SD memory cards or appropriate batteries. This may lead to damages to the recorder and endanger the patient.

**Note**

- Use only a Norav Certified SD card for Recording.
- It is the end user's responsibility to properly configure the NR recorder with settings that are compatible with their ECG analysis software.
- False positive and false negative pacer detects may occur when using Pacer Detect.
False positives - may result from poor electrode connection to the patient or a large amount of electrical interference from nearby objects.
False negatives - may occur with pacers that are bipolar because of a weak pacer pulse signal at the patient's skin.
- The recorder is not designed for emergency purposes (intensive medical). It is only designed to record the ECG and/or heart rate.

Controls and Indicators

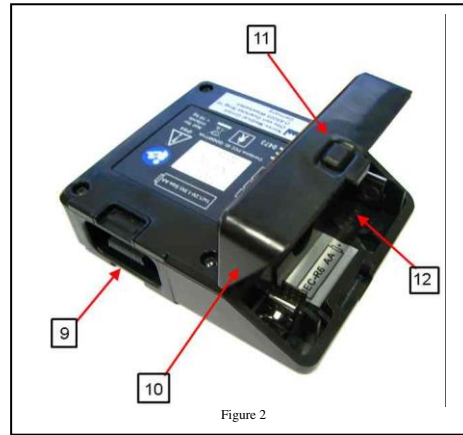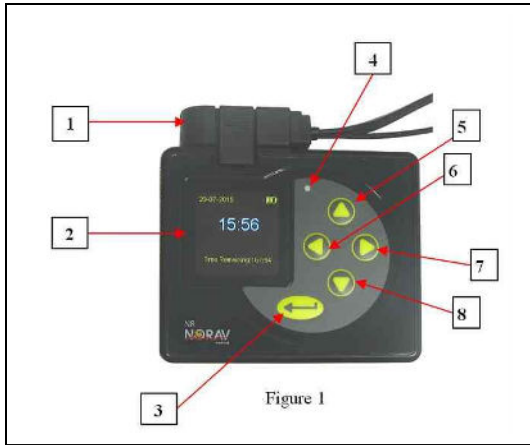

Element	Description
1	Patient ECG Cable connector
2	Screen to display feedback from the recorder
3	Enter, Event button
4	Green led Indicator , Voice recorder microphone
5	Up button
6	Left button
7	Right button
8	Down button
9	ECG cable connector slot
10	Battery and SD Flash card compartment door
11	Battery and SD Flash card compartment cover latch
12	Battery and SD Flash card compartment


Memory Card (SD card)

(Skip this step when use models NR-1207-E and NR-314-T.)

The SD (Secure digital) card is a memory card that is formatted (see note below) exclusively for recording biological information. This card is an IC card composed of electrically erasable, non-volatile IC memory referred to as “flash memory”. This offers the advantage that the data contained in the IC card is retained while the power is shut down, thereby eliminating the need for backup batteries.



Open battery compartment cover by moving Left and Up the battery compartment cover latch.

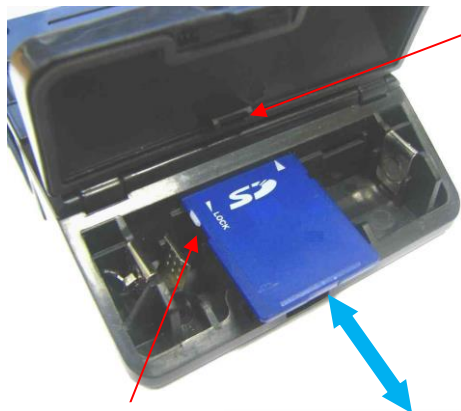

Memory card Retainer

The memory card slot is a so-called "push-push slot".


In order to insert the memory card into the device, push the card into the slot until it locks in place.


To remove the memory card, push the card 1-2 mm into the slot to release the locking catch.



The battery must be removed prior to inserting or removing the SD card.

Battery compartment cover has a memory card retainer used to protect the card from falling out of its slot during recording.

Write-protect notch, Unlocked state shown

 Caution	<ul style="list-style-type: none"> • The recorder is mechanically protected from an incorrect insertion of the memory card. Do not force the card into the slot. • Using the memory cards with other instruments (digital cameras, MP3 players, etc.) can lead to incorrect functioning and/or data loss. • If memory card is not completely locked inside its slot, the card retainer (part of battery compartment cover) will not allow to close the cover. Do not push the cover when closing with force; it can damage the card and/or the card slot.
---	--

 Note	<ul style="list-style-type: none"> • When looking at the SD card from the top, on the left side, there may be a write-protection notch. If notch is not in Unlocked state, slide the tab upward (Toward the contacts) to declare the card read/write enabled. • If the storage space runs out during a recording, the recording is stopped automatically and the instrument switches off.
--	---

 Note	<ul style="list-style-type: none"> • Use only a Norav Certified SD card for Recording. • The NR recorder supports only SD cards formatted as follows: FAT(FAT16) with cluster size = 64KB for SD cards ≤ 4G or FAT32 with cluster size = 64KB for SD cards > 4G 	
--	--	---

Main Battery

The NR is powered by one 1.5 volt AA Alkaline battery (IEC-LR6), one 1.2 volt AA rechargeable Nickel-Metal Hydride (NiMH) battery (IEC-HR6), or one 1.5 volt AA Li-FeS2 Lithium battery (IEC-FR6). Although battery life may last longer than a recording, batteries should not be re-used for a second patient. After one use, they should be disposed of following local ordinances.

Insert Battery



Insert a fresh AA battery as indicated in illustration, be sure to first insert from the negative terminal. Pay special attention to the correct polarity of the battery



As indicated in the illustration, close battery compartment cover and press on it until latches into the base part.



Caution

- Check that recorder settings showing a correct Battery type in the setup of the recorder.




Caution

- Do not leave battery in the recorder for extended periods (more than two weeks) when the recorder is not in use.
- If you use rechargeable batteries, the battery recharger should be kept out of the patient environment and hook-up area.
- Dispose of used batteries carefully, using environmentally friendly methods wherever possible following the state's recycling laws or your facility's recycling policy

RTC Back up Battery

The NR real-time clock is maintained by an internal rechargeable lithium cell, charged during recording from the main battery. With a full charge, the clock is maintained for at least 4 months after the main battery is removed. The clock cell is not replaceable by the user, and in the case of suspected failure the NR should be returned to Norav for service.

Electrode Application



Note

Many ECG adhesive electrodes are suitable for use. As ECG electrodes from different manufacturers have different electrical properties, the choice of ECG electrodes can considerably affect the measurement results and quality. Ensure that only high-quality electrodes are used. Wet gel electrodes are recommended.


Always refer to the ANSI/AAMI EC12:2000 Standard for safety, performance, and labeling requirements for the disposable electrodes, and guidelines for reliable patient connections.

Prepare the patient's skin prior to applying the electrodes. Skin is a poor conductor of electricity, so skin preparation is important in achieving good electrode-to-skin contact.

- If necessary, clip hair at the electrode sites (or shave sites, if needed).
- Clean and abrade the skin at the electrode sites to remove oil and dead skin.
- Wash the skin thoroughly with soap and water.
- Dry the electrode placement sites.

Attaching the electrodes

- Attach the leads to the electrodes before placing them on the patient.
- Apply the electrodes by peeling them, one at a time, from the protective backing and sticking them firmly to the patient's skin.
- The electrodes should be placed over bone at each of the sites.
- The offset connector tab should be positioned in the same direction as the lead wires, towards the equipment.
- Place the electrode on the skin by gently pressing around the edge. For wet gel always avoid pressing down the centre of the electrode. If in doubt refer to the directions on the reverse of the pouch.



If you use lead lock or clip lock electrodes, be sure to use the lock or clip to relieve stress on each lead wire.

Otherwise, tape each lead wire into a stress loop to help prevent movement of the electrode.



WARNING

- As you attach electrodes, be careful to not let any unattached electrode come in contact with other conductive objects, including ground.
- Leave 1.5 meters (5 feet) of open area around the patient during recorder hookup and removal.
- Do not connect external devices to the recorder. Connect patient lead wires only to the patient electrodes
- Keep the recorder and patient cable clean, especially the components that touch patients.
- Do not use electrodes for adults on children.
- Before each recording and before attaching sensors or electrodes to the patient, check the casing and the ECG patient cable for damage which may have occurred, for example, due to mechanical overload, falling from a great height or wear and tear (chafed patches on the cable). Do not use the instrument or the cable if you detect cracks, melted areas or any other signs of damage to the cable or housing.




Caution

- Verify that dates on applicable accessories have not expired.
- ECG electrodes can cause skin irritation. Examine the skin for signs of irritation or inflammation and avoid placement of the electrode in those areas. If skin irritation occurs during the procedure advise the patient to remove the electrodes and contact the health service provider as soon as possible.







Electrode Placement

Suggested electrode placements are shown in the diagrams below. However, it is up to the physician to make the final placement determination. The recorder's ECG display screen or Computer Analysis System that used Bluetooth communication can be used to verify a proper patient hookup.



Caution

- Do not rely on the recorder LCD display as a diagnostic tool.

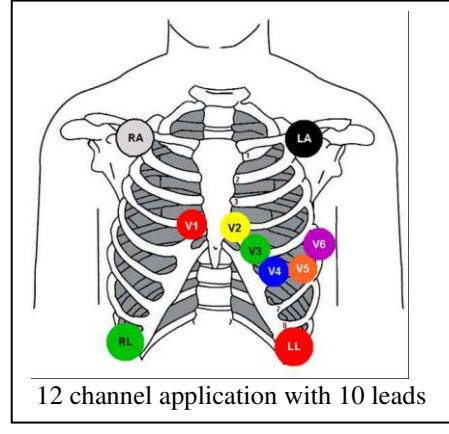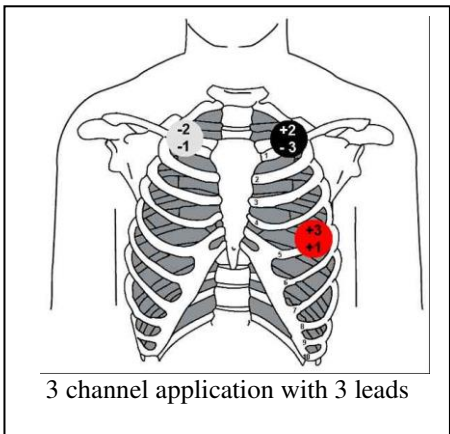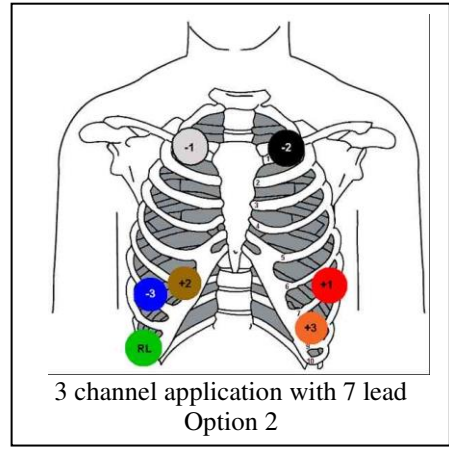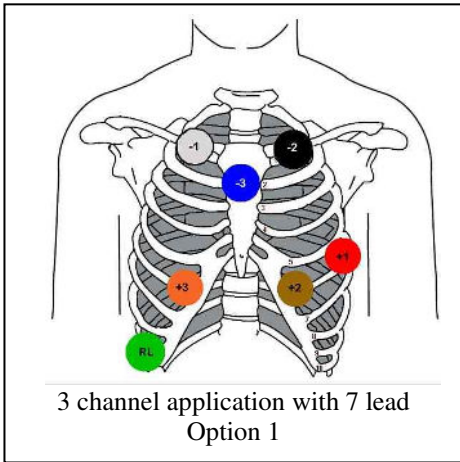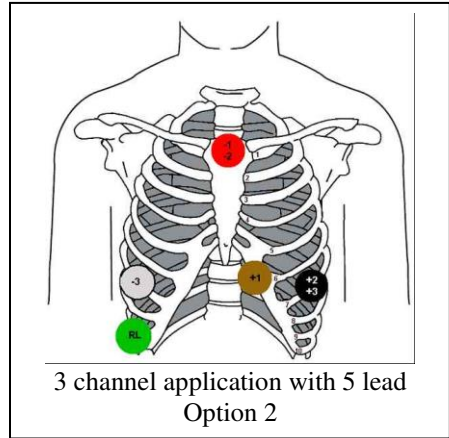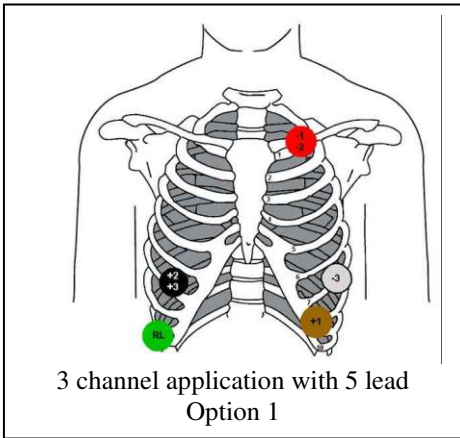

Patient Cable Connection



Connecting:

Insert the Patient ECG Cable connector into ECG cable connector slot of the NR unit, as shown on the picture. Make sure to insert the Cable connector until there is no space between the Cable connector and the unit. Make sure that two latches of the Cable connector are latching with the unit.

Disconnecting:

Remove the Patient ECG Cable connector by squeezing the two side latches on the head of the Cable connector and pulling away from the connector slot of the NR unit.



Caution

- Be careful not to connect the Patient ECG Cable connector upside down or at an angle into the ECG cable slot on the NR unit. This may result in damage to both the Cable connector and the ECG Cable input slot of the unit.
- Do not insert into the ECG Cable slot on the NR any other than the Patient ECG Cable connector. Damage can result to the both the ECG Cable slot input connector and Patient ECG Cable connector.
- Always check the presence of sealing O-ring on Patient ECG Cable connector and its quality. O-ring sealing protects the NR unit against ingress of splashing water when the Patient ECG Cable connector is fully fitted into the unit.
- During recording, make sure that the cable lead wires are not caught by the moving parts of a machine or sport equipment. This could lead to damage or injury (e.g. if loops are formed in the cable lead wires).
- NEVER pull on the cable itself because this can easily break the wire inside the insulation. Pulling on the cable also can cause a noisy and intermittent ECG recording.




Note

NR hardware includes Cable connected sense. If NR will not detect connected Cable, it will display warning message with buzzer beep and show diagram of unit with not connected Cable connector.

Screen Navigation

The NR recorder uses various menus to set preferences and enter patient information. Four keys, left, right, up and down, are used to navigate the menus. The enter key is used to make a selection of a highlighted item. Recorder involves a simple sequential procedure comprising: Record Mode Setting, Date & Time Checking or Setting, Patient Identification Entry, ECG signal quality Checking and Start Recording. The user interacts with the recorder through different LCD screens and five push-buttons.



- To prevent possible damage to the keypad, do not use sharp or hard objects to depress keys.

Caution

Brief descriptions of recorder screens

Screen	Description
Main	Displays Current datetime, Main battery level, and following Menu items : <ul style="list-style-type: none"> • Patient Data <i>(Display Patient data – ID or Name)</i> • Voice Recording <i>(Record operator voice message - up to 20seconds)</i> • Recording Settings <i>(Display enabled recording settings)</i> xxxH = Record time in hours \E = Event button enabled \P = Pacemaker detection enabled \R = Respiration enabled \A = Acceleration sensor enabled
Settings	Displays Menu items: <ul style="list-style-type: none"> • Patient Settings <ul style="list-style-type: none"> ➤ ID <i>(Change via Virtual keyboard screen)</i> ➤ First Name <i>(Change via Virtual keyboard screen)</i> ➤ Last Name <i>(Change via Virtual keyboard screen)</i> ➤ Birthday <i>(Change via Virtual keyboard screen)</i> ➤ Clinic ID <i>(Change via Virtual keyboard screen)</i> ➤ Display Format Patient ID, Clinic ID, Name <i>(Select patient data field to display on the Main screen)</i> • Record Settings <ul style="list-style-type: none"> ➤ Record Time 24,48,72,96,120,168, 336 hr <i>(336 hours option is limited to 3 channel mode with 3, 4 , 5, 7 lead cable , 250 sample rate and Lithium battery only)</i> ➤ Sample Rate (of ECG) 250,500,1000<i>(samples per second)</i> ➤ Pacemaker detection ON or OFF <i>(OFF by default. Once turned ON remains active within the current recording only)</i> ➤ Accelerometer ON or OFF ➤ Respiration ON or OFF <i>(always OFF when Pacemaker detection is ON)</i> ➤ Diary OFF , Event button, Symptom list, Voice note <i>(in Holter/Holter+ mode)</i> <ul style="list-style-type: none"> ■ Event button - Save Event for each button press ■ Symptom list – Select a symptom from list on the Display ■ Voice note - Record a Voice note ➤ Voice note ON or OFF <i>(When ON - allow to record a Voice note) (for NR-1207-3 model in ECG+ mode)</i>

Brief descriptions of recorder screens (continue)

Screen	Description
Settings (<i>continue</i>)	<ul style="list-style-type: none"> • System Settings <ul style="list-style-type: none"> ➢ Date\Time <ul style="list-style-type: none"> ■ Date (Month,Day,Year) ■ Date Format (MM/DD/YYYY, YYYY/MM/DD, DD/MM/YYYY, YYYY/DD/MM) ■ Time (Hour and Minute) ■ Time Format (12 or 24 hr) ➢ Display <ul style="list-style-type: none"> ■ Contrast (20-90%) ■ Rotation (0, 90, 180, 270 deg.) ➢ Battery <ul style="list-style-type: none"> ■ Alkaline ■ NiMH ■ Lithium ➢ Language <ul style="list-style-type: none"> ■ English ■ Español ■ Deutsch ■ Français ■ Italiano ■ Português ■ Nederlands ■ Polski ■ Русский ■ Ελληνική ■ Türk ➢ Mode (for NR-1207-3 model only) <ul style="list-style-type: none"> ■ Holter ■ Holter+ ■ ECG ■ ECG+ • Save as default (Press Enter to save as default current settings) • About (Press Enter to see recorder information – Model, Serial number etc.)
Lead check	Displays the connection status of each lead
ECG CH1,CH2,CH3 or I,II ... V6	<p>Displays the ECG signal in real time. Pacer pulse marks and the gain setting are also displayed.</p> <p>To change the gain use up\down buttons of the keypad, gain settings are (0.5,1.0,2.0,4.0,8.0)</p> <p>The gain setting is the same for all channels and only affects information displayed on the screen. The recording will always be made at the 1.0x gain setting.</p> <p>The display grid size at 1.0x gain settings equals to 10 mm/mv (two grid boxes=1 mv).</p> <p>If <i>Pacemaker Detection</i> is turned on, pacer pulse marks are displayed below the trace to indicate each detection of a pacer pulse.</p>
Start	After configuring or reviewing all the settings, select the start screen and press <i>Enter</i> . This will start the recording. During recording, the recorder displays the current time and time remaining to record.
Info	During recording NR recorder will display the date, current time, battery level indicator and time remaining for the recording.

“Main” menu screen - explanation of menu navigation by using keypad buttons almost the same for the others menu screens.

The screenshot shows the main menu with the following elements and callouts:

- Menu Item[1]: Patient ID**: Points to the 'Patient ID:' label.
- Recorder Date&Time**: Points to the date and time '03-08-2015 10:00'.
- Main Battery Indicator**: Points to the battery level icon.
- Menu Item[2]: Voice Record**: Points to the 'Voice Record' option, which is highlighted. The callout text says: "Selected Item is highlighted in current Menu Screen. Navigate to above or below menu Item by using up/down buttons of the keypad."
- Menu Item[3]: Recording settings**: Points to the '168H / E' value. The callout text says: "Record Time = 168Hr, Event Button = On".
- Help line text meaning:**: Points to the 'Settings' and 'Lead Status' options. The callout text says: "Navigate to the Next/Previous Menu screens by using left/right buttons of the keypad".
- Help line text meaning:**: Points to the 'Press [Enter] to start' instruction. The callout text says: "To start Voice Recording Press Enter button of the keypad".

“Virtual Keyboard” menu screen (alphabet layout with lower case shown), used to enter Patient Data like ID, First Name etc. Use up/down/left/right buttons of the keypad to navigate via the virtual keyboard screen items.

The screenshot shows the virtual keyboard screen with the following elements and callouts:

- Entered characters**: The string 'Thomas_' is shown at the top. The callout text says: "This line shows entered characters from the virtual keyboard. This character string will be saved if select item 'Save' at the bottom of the screen and pressing Enter button of keypad."
- Selected character**: The character 's' is highlighted. The callout text says: "Selected character is highlighted – press Enter button of keypad to insert it to the string at line above. Navigate with up/down/left/right buttons of the keypad to select different character".
- Virtual keyboard control icons line**: A row of icons for keyboard layout selection. The callout text lists:
 - Select - upper or lower case alphabet keyboard layout
 - Select - Space character
 - Select - Backspace character
 - Select - Numeric keyboard layout
 - Select - Alphabet keyboard layout
 - Select - Extended alphabet keyboard layout
 Note: Alphabet and extended alphabet layout depends on system language of the recorder.
- Navigation**: 'Save' and 'Cancel' buttons are at the bottom. The callout text says: "Navigate here with up/down/left/right buttons of the keypad to Save or Cancel the entered string at the top of the screen".

Common Workflow

Holter mode (for NR-302/314/1207/1207-3 models)

A basic workflow for “classic” Holter recording procedure.

- Prepare recorder.
- Enter patient information.
- Hookup patient
- Check ECG leads quality.
- Start recording.
- While recording continues enter diary events by patient.
- When patient bring the recorder back stop the recording.
- Download the ECG recording file to the computer.
- Preview/Analyze the ECG in Holter software interface.

Holter+ mode (for 1207-3 model only)

Advanced workflow allowing to acquire the ECG traces online while Holter recording is continues.

- Prepare recorder.
- Enter patient information.
- Hookup patient
- Check ECG leads quality.
- Start recording
- Acquire the live ECG every time when it is necessary
(*patient must be near to the acquisition workstation*)
- While recording continues enter diary events by patient (optional).
- When patient bring the recorder back stop the recording.
- Download the ECG recording file to the computer.
- Preview/Analyze the ECG in Holter software interface.

ECG mode (for NR-314-T/1207-E/1207-3 models)

Standard workflow for PC-ECG acquisition.

- Prepare recorder.
- Hookup patient.
- Check ECG leads quality.
- Run the PC-ECG or Mobile ECG software application and enter patient information.
- Acquire the live ECG.

ECG+ mode (for 1207-3 model only)

Advanced mode for record continuously the ECG traces in the NR recorder memory independently to live ECG is acquiring or not. Allows to store ECG records for more than one patient on the same memory card.

- Prepare recorder.
- Enter the patient information.
- Hookup the patient.
- Check ECG leads quality.
- Start ECG recording to the NR device memory card.
- Every time when it need - launch the PC-ECG or Mobile ECG software and acquire the live ECG.
- At the end testing of current patient – stop (pause) the ECG recording.
- Hookup the next patient and then continue the recording in the NR memory card.
- When NR memory card is filled – download the full disclosure ECG data to the computer.

ECG Recording Detailed Instructions

Starting New test

1. Prepare Recorder

- Open NR recorder battery compartment door.
- Insert an SD card into recorder. (*Skip this step when use models NR-1207-E and NR-314-T.*)
- Insert a new battery and close the battery compartment door.
(*Green led of the keypad will start flashing once per second*)
- Prepare the patient (*the patient should already be connected to the electrodes and patient leads*) and connect the ECG cable connector to the recorder unit.
- Turn on the recorder by pressing the *Enter* button of the keypad.

2. Enter Patient Information (for Holter, Holter+ and ECG+ mode)

If an SD card was preinstalled with the Patient Data\Recording Settings file, this information will be loaded by the recorder. Check Patient data (*ID, Name etc.*) using the LCD screens. If Patient data is missing or wrong enter Patient data using the LCD menus screens and unit keypad.

Alternatively if using model with voice record enabled; the patient data can be recorded using voice record option in the “main” screen. In this way, the measurement can still be clearly identified. Recording is possible for up to 20 seconds. Make sure that the microphone (*Green led on keypad*) is close to your mouth when recording and that you speak at a normal volume.

Check recording settings, change them if required.

3. Check ECG Leads

Check the signal quality and amplitude of each channel via ECG screen menus.

If ECG signal quality does not show satisfactory ECG waveforms, reposition electrode sites using brand new electrodes and techniques described above in this manual. Instruct the patient to stand, sit, and lie while verifying the ECG signals. Instruct patient to walk in place. Verify no artifact or muscle noise is displayed on the recorder LCD screen. Otherwise, check stress loops and re-prep hookup sites with brand new electrodes.

4. Start Recording (for Holter, Holter+ and ECG+ mode)

- The ambulatory ECG recording is ready to begin. Access the “Start” screen. Press the *Enter* button of keypad to start recording.
- The LCD will show “Recording” screen. During recording the NR recorder will display the date, current time, battery level indicator and time remaining for the recording. If no button has been pressed for some time, the screen goes blank; and every time a button is pressed, the LCD will show “Recording” screen for a short time.
- Place recorder into pouch or holster and secure on the patient. All equipment, except the electrodes and a portion of the lead wires, should be over at least one layer of clothing so that it is not in direct contact with the patient’s skin. Orient the recorder on the patient so that the *Enter (Event)* button is accessible and the LCD is visible.
- Advise the patient to not expose the recorder or electrodes to any wet environment; in addition, they should not shower, bathe, or swim while wearing the recorder.
- Instruct the patient on how to use the *Enter (Event)* button to indicate symptomatic events or activities of interest during the Holter test. The patient may also be given the opportunity to enter a diary at the time of the event. They should use the up/down arrows to choose the most appropriate entry. Alternatively if using model with voice record enabled; the patient can use the voice record to enter a diary.

Acquire ECG On-line (for Holter+, ECG and ECG+ mode)

In Holter+ recording mode the NR-1207-3 recorder is able to transmit the live ECG traces online.

To acquire the live ECG waveforms online use the Resting ECG software application of PC-ECG 1200 package or the Mobile ECG application for Android OS. Refer to the appropriate user manual accordingly.

Enter a Diary Event (for Holter, Holter+ mode)

Press and hold the Enter button on the NR recorder front panel. Depending to the configuration setting - might follow require to select the symptom from the list or add a voice note.

Add a New Patient Marker (for ECG+ mode only)

While the ECG Recording is running (the 'REC' label is flashing on a Lead Check screen)
- press and hold the Enter button on the NR recorder front panel.
The patient counter will be increased and (if enabled) the voice note can be added at this time.

Stop/Pause/Restart the ECG Recording (for ECG+ mode only)

While the ECG Recording is running (the 'REC' label is flashing on a Lead Check screen)
- press and hold simultaneously both left and right arrow buttons on the NR recorder front panel.
When the record control menu appears select the needed command from the list:

- “**Stop ECG**” - to pause the ECG recording (finish for current patient).
- “**Overwrite Record**” - to clean the memory card and restart the ECG recording (*previously recorded ECG traces will be erased from the NR recorder memory!*)
- “**Shutdown**” - to switch the NR recorder OFF before to remove the memory card and download the ECG recording to the computer.

To Stop Holter Recording (for Holter and Holter+ mode)

When the set recording duration has been reached or if the battery capacity is low, the recorder switches off automatically. The recording can be stopped at any time by pressing and holding both keypad buttons (left and right) for 3 seconds.

Data Download


When the session is complete (completed by a trained medical technician) the ECG record data is available for analysis.

- 1) Remove the electrodes from the patient.
- 2) Remove the battery from the recorder.

The user has two options to analyze the captured ECG data by Computer Analysis System:

- 1) Remove the memory card from the recorder. Insert the memory card into the card reader of the Computer Analysis System and transfer the ECG data according to the manual for the Computer Analysis System.
- 2) The user also has the option (if enabled) to download the recording on the memory card via USB without having to remove the card from the recorder. Start by removing the patient cable, replace it with the USB cable and confirm that the card is still in the recorder. Attach the other end of the USB cable to any available USB port on a computer. The recorder is now a card reader and can be accessed similarly as any removable disk drive would be.

Once the data transfer is complete, erase the ECG record data from the memory card.
The memory card is now free to be used for the next patient.

**Note**



- The NR recorder with installed battery and SD card, turned ON and ECG cable connector connected to the unit; and is left for 10 minutes without pressing any button of keypad, will start the test automatically (*for Holter and Holter+ modes*). This feature of the device shall eliminate the risk that the operator forgets to start the test.
- The NR recorder with installed battery and SD card, turned ON and ECG cable connector connected to the unit; and detects a recording saved on the memory card which has not yet been downloaded by the Computer Analysis System, will show warning message screen and will offer an option to erase the old record and prepare the device for a new record on the same memory card.
- If the batteries run flat during a recording, it is necessary to replace them with fully charged batteries within 1 hour. If the batteries are replaced in time, the NR recorder will resume the recording. However, the device will not continue in the test, if the batteries are not replaced in time. The data recorded before the battery runs flat are stored in the memory card and can be freely accessed and analyzed after download by Computer Analysis System.
- The recorder will only allow you to select settings for a recording what will fit on the SD flash card. There is a relationship between the record time, sample rate, and number of channels. By choosing a higher value in one setting, you may have to choose a lower value than you want in another setting. It is best to first set the lowest setting you desire, then the second highest, and so on.

Maintenance and Cleaning



Reprocessing methods for reusable items

The following tables summarize the required post-test reprocessing procedures for each reusable item.

ECG Device surfaces


Level of Reprocessing	Low-level disinfection
When	Immediately after use
Pretreatment	Wipe with a moist sponge or paper towel
Manual Cleaning 	Wipe the surface with a soft cloth dampened with a solution of warm water and mild dishwashing detergent or ordinary alcohol-free hand soap. Dispose the soft cloth.
Disinfection 	Repeat manual cleaning. Wipe device surface with alcohol wipes. Dispose the soft cloth.
Drying	Air dry or wipe all surfaces with a dry clean cloth or paper towel.
Note	Do not clean in Ultrasonic baths.

Patient Cables\Leadwires

Level of Reprocessing	Low-level disinfection
When	Immediately after use
Pretreatment	Wipe with a moist sponge or paper towel
Manual Cleaning 	Wipe the surface with a soft cloth dampened with a solution of warm water and mild dishwashing detergent or ordinary alcohol-free hand soap. Dispose the soft cloth.
Disinfection 	Repeat manual cleaning. Wipe device surface with another soft cloth moistened with 70% isopropyl alcohol\ethanol. Dispose the soft cloth.
Drying	Air dry or wipe all surfaces with a dry clean cloth or paper towel.
Note	Do not clean in Ultrasonic baths.


Sterilization for Patient Cables\Leadwires

Sterilization Method	Ethylene oxide (EtO)
When	Only when necessary as specified by your facility.
Pretreatment	Prior to sterilizing cables\leadwire should first be cleaned. To avoid long term damage of cables\leadwire.
Sterilization procedure	The product may only be sterilized with ethylene oxide (EtO) at a maximum temperature of 50 °C (122 °F).
After Sterilization	After sterilization, cables must be safely and thoroughly ventilated before handling or use. Recommendation of an aeration time of 12 hours minimum to dissipate residual EtO in the cable below 250 ppm.
Note	It is important to check that there are no alterations to the components or overall functioning of the product in sterilization. At first sight of alteration the product must be replaced.
Validation	The validation of the subsequent sterilization is the responsibility of the user.
Note	Do not autoclave cables\leadwires. Do not sterilize by irradiation or steam. Do not clean in Ultrasonic baths.



Caution

- Remove the battery before cleaning the NR recorder.
- Take care to prevent chemicals/liquids from entering the connectors or internal part of the recorder.
- The battery contacts should not come in contact with soap or water.
- Do not polish the housing with abrasive or chemical cleanser.
- Use of alcohol, acetone, Alkyl Dimethyl Benzyl ammonium chlorides or a methyl ammonium chloride is NOT recommended to clean the recorder unit and holster. Use of alcohol or acetone on lead wires could cause the lead wires to stiffen and the insulating plastic to crack. Use of a methyl ammonium chloride (commonly found in many consumer wipes) on the recorder unit and holster could cause the plastic to deteriorate.



Note

If liquid penetrates the device, i.e. during cleaning or recording, this may interfere with correct functioning. Switch the recorder OFF, remove the patient cable, the memory card and the battery. Leave the recorder in a warm, dry room with the battery door open for 48 hours. If the functioning is still affected, contact the contact customer support.

Maintenance:

Before using the NR recorder, execute the check of the unit in accordance with the check procedure. In case that any rejected items are found as a result of the check, it will be totally judged as rejection. Take the corrective measures as the rejected items. Use the recorder after all the items become accepted. Unit check shall be performed by each medical institution, or by Norav personnel, representative agent, or an authorized third party. For more details, do not hesitate to consult your dealer or Norav Medical personnel.

Details of the check	Check Method	Criteria
SD card	Visually check for scratches and damage.	Must be free from scratches and damages.
Operation manual	Check that the operation manual is kept in a predetermined place.	Should be kept in a predetermined place.
Cracks and distortion of the recorder enclosure	Visually check the recorder enclosure for cracks and distortion.	Must be free from cracks and distortion.
Battery compartment	Check whether dirt or hair is not accumulated between the battery compartment and its door	Must be free from dirt or hair.
Keypad buttons	Check whether the keypad buttons have tactile feedback when pressed	Must get tactile feedback.
Battery contacts in the battery compartment	Visually check the battery contacts for strain, skew, and corrosion.	Must be free from strain, skew, and corrosion.
Battery compartment door latch	Check spring loaded in the battery door latch.	Spring must be loaded.

Storage

Before storage, make sure to remove a main battery and a SD card from the NR recorder and close the battery compartment door tightly. Store the recorder in the provided storage case.



Caution

- Store the NR recorder in an area free from water or humidity
- Take care to avoid areas subject to high humidity, poor ventilation and direct sunlight; store the NR recorder in an area free from any adverse effects of surrounding air containing dust, sodium, and sulfur.
- Do not store the NR recorder in an area where chemicals are kept or which is exposed to chemical fumes or vapors.

Service

If there is a problem with the NR recorder, review the Troubleshooting section for a listing of problems and solutions. If additional assistance is required, contact customer support via phone, fax or e-mail listed in this manual. Call customer support before returning a recorder to make shipping arrangements.

All repairs on products under warranty must be performed or approved by Norav Medical. Unauthorized repairs void the warranty. In addition, whether or not covered under warranty, any product repair shall exclusively be performed by Norav Medical certified service personnel.

When calling, please be prepared to provide:

- Product name and complete description of the problem.
- Serial number of your product.

In case a return cannot be avoided, the representative will record all necessary information and will provide a Return Material Authorization (RMA) number, as well as the appropriate return address. An RMA number must be obtained prior to any return.

If you have to return goods for service, follow these recommended packing instructions:

- Remove all cables, sensors, and ancillary products (as appropriate) before packing, unless you suspect they are associated with the problem.
- Wherever possible use the original shipping carton and packing materials.
- Include a packing list and the Norav Return Material Authorization (RMA) number.

It is recommended that all returned goods be insured. Claims for loss or damage to the product must be initiated by the sender.

Calibration

The device does not need any calibration.

Troubleshooting

Symptom	Solution
No display or recorder does not power on	<ul style="list-style-type: none"> ■ Ensure battery is inserted with correct polarity. ■ Install a new AA battery.
Low battery (<i>message</i>)	<ul style="list-style-type: none"> ■ Install a new AA battery. ■ Inspect battery compartment, clean contacts if necessary.
No Cable (<i>message</i>)	<ul style="list-style-type: none"> ■ Ensure patient cable (lead set) is connected to the recorder. The recorder will not pass the screen unless a cable is connected. ■ Check that the recorder sided connector is not damaged. Check that the cable connector pins are not broken or bent / damaged.
Noise artifacts on ECG signal	<ul style="list-style-type: none"> ■ Ensure you have prepared the patient's skin according to the instructions. ■ Ensure the electrodes are properly applied to the patient. ■ Ensure the leads are making proper contact with the electrodes. ■ Replace the Patient ECG cable.
Lead OFF (<i>message</i>)	<ul style="list-style-type: none"> ■ Ensure you have prepared the patient's skin according to the instructions. ■ Ensure the electrodes are properly applied to the patient. ■ Ensure the leads are making proper contact with the electrodes. ■ Replace the Patient ECG cable.
SD Card Error (<i>message</i>)	<ul style="list-style-type: none"> ■ Ensure the memory card is Norav Certified. ■ Ensure the memory card is not write protected (small switch on the SD Card) ■ Reformat the memory card or replace the card with a new Norav certified memory card.
Previous recording found (<i>message</i>)	<ul style="list-style-type: none"> ■ Download the ECG data with Computer Analysis System, or delete it from the SD card using left and enter buttons.
Set Date/Time (<i>message</i>)	<ul style="list-style-type: none"> ■ The internal battery that runs the real time clock may not be fully charged. This battery is built into the recorder and is not user replaceable. It is recharged every time you insert an AA battery. If the recorder is unused for an extended period of time, the internal battery can become discharged. To fully recharge the internal real time clock battery, insert a fresh AA battery into the recorder and let the recorder charge, for 12 hours.
SD card too small (<i>message</i>)	<ul style="list-style-type: none"> ■ Check that Record Settings screen is set for the desired number of hours. Memory card has only enough memory capacity to run for the number of Hours which are available as valid selections in the Record Settings menu.

Technical Specifications

	Conditions	min	typical	max	Unit
Dimensions					
Width			92		mm
Height	Without ECG cable		75		mm
Depth			23		mm
Weight	Without battery		103		g
Ingress protection against water	With ECG cable connected, Battery door closed and sealing installed.		IP22		
ECG					
Channels		3		8	
Input impedance		>10			MOhm
CMRR		>90			dB
Frequency Response HPF	Recording		0.05		Hz
Frequency Response LPF	Recording	65		260	Hz
Dynamic range	Recording, peak to peak		10		mV
A/D bit Resolution	Recording		12		bit
Sampling rate	Recording	250		1000	Hz
Pacemaker detection	Analogue detection on 2 channels				
	Amplitude		2	700	mV
	Width		0.1	2	ms
Accelerometer					
Channels			3		
Dynamic range	Recording, peak to peak		4		g
Respiration					
Channels	Sensing electrodes ch1+,ch1-		1		
Excitation current			27.3		uA
Excitation frequency			64		kHz
Power					
Supply voltage	1x AA battery	1.0	1.5	2.7	V
Internally occurring voltage			2.8	13	V
In RMS current during recording	Vbatt=1.5V	10		150	mA
Ambient conditions					
Ambient temperature	Storage	-20		+60	°C
	Operation	+10		+45	°C
Humidity (non-condensing)	Storage	10		95	%RH
	Operation	10		95	%RH
Atmospheric pressure	Storage	700		1060	hPa
	Operation	700		1060	hPa

Conformance to Regulatory Standards	IEC 60601-1, IEC 60601-1-2, IEC 60601-2-25, IEC 60601-2-47, IEC 60601-1-11
Classification	Type-BF applied part (NR-314, NR-302, NR-1207), Defibrillation-Proof Type CF Applied Part (NR-1207-3, NR-2017-E, NR-314-T), Internally powered equipment, Equipment for continuous operation
Communication	USB 2.0 HS, Bluetooth 2.1+EDR Class1

ECG Cables and Accessories

Item	Part Number	NR Compatibility	Application	Defib. protected
ECG Cables				
3 Lead Patient Cable, Snap, AHA	C3-S-U-EI	302, 314, 1207, 1207-3	Holter	No
4 Lead Patient Cable, Clip, AHA	C4-C-U-EI-07	314-T, 1207-3, 1207-E	Telemetry, Stress	Yes
4 Lead Patient Cable, Clip, IEC	C4-C-E-EI-07	314-T, 1207-3, 1207-E	Telemetry, Stress	Yes
5 Lead Patient Cable, Snap, AHA	C5-S-U-EI	314-T	Telemetry	No
5 Lead Patient Cable, Snap, AHA	C5-S-U-EI	302, 314, 1207, 1207-3	Holter	No
5 Lead Patient Cable, Clip, IEC	C5-C-E-EI-07	1207-3, 1207-E	Rest	Yes
5 Lead Patient Cable, Clip, IEC	C5-C-E-EI-08	1207-3, 1207-E	Rest	Yes
5 Lead Patient Cable, Clip, AHA	C5-C-U-EI-07	1207-3, 1207-E	Rest	Yes
5 Lead Patient Cable, Clip, AHA	C5-C-U-EI-08	1207-3, 1207-E	Rest	Yes
7 Lead Patient Cable, Snap, AHA	C7-S-U-EI	302, 314, 1207, 1207-3	Holter	No
7 Lead Patient Cable, Snap, IEC	C7-S-E-EI	302, 314, 1207, 1207-3	Holter	No
10 Lead Patient Cable, Snap, AHA	C10-S-U-EI	1207, 1207-3	Holter	No
10 Lead Patient Cable, Snap, IEC	C10-S-E-EI	1207, 1207-3	Holter	No
10 Lead Patient Cable, Clip, AHA	C10-C-U-EI-07	1207-3, 1207-E	12-lead ECG	Yes
10 Lead Patient Cable, Clip, IEC	C10-C-E-EI-07	1207-3, 1207-E	12-lead ECG	Yes
10 Lead Patient Cable, Banana, AHA	C10-B-U-EI	1207-3, 1207-E	12-lead ECG	Yes
10 Lead Patient Cable, Banana, IEC	C10-B-E-EI	1207-3, 1207-E	12-lead ECG	Yes
Accessories				
USB 2.0 HS Cable, 1.5m	USBA-1.5M-EI	302, 314, 1207, 1207-3		
Recorder Holster	NR-HOL	302, 314, 1207, 1207-3, 1207-E		
Recorder Pouch	NR-P	302, 314, 1207, 1207-3, 1207-E		
Certified NR SD Memory Card 2GB	NR-2G-SD	314, 1207, 1207-3		
Certified NR SD Memory Card 512MB	NR-512M-SD	302		

Electromagnetic Emissions and Immunity Information

Refer to the following tables for specific information regarding NR recorder compliance to IEC 60601-1-2.


Table 1: Electromagnetic Emissions

Emissions Test	Compliance	Electromagnetic Environment—Guidance
<i>This device is intended for use in the electromagnetic environment specified below. The customer and/or user of this device should ensure that it is used in such an environment.</i>		
RF Emissions CISPR 11	Group 2	This device must emit electromagnetic energy in order to perform its intended function. Nearby electronic equipment may be affected.
RF Emissions CISPR 11	Class B	This device is suitable for use in all establishments, including domestic and those directly connected to the public low-voltage power supply network that supplies buildings used for domestic purposes.
Harmonic Emissions IEC 61000-3-2	N/A	
Voltage Fluctuations/Flicker Emissions IEC 61000-3-3	N/A	

Table 2: Electromagnetic Immunity

Immunity Test	IEC 60601 Test Level	Compliance Level	Electromagnetic Environment—Guidance
<i>This device is intended for use in the electromagnetic environment specified below. The customer and/or user of this device should ensure that it is used in such an environment.</i>			
Electrostatic Discharge (ESD) IEC 61000-4-2	±6 kV contact ±8 kV air	±6 kV contact ±8 kV air	Floors should be wood, concrete, or ceramic tile. If floors are covered with synthetic material, relative humidity should be at least 30%.
Electrical Fast Transient/Burst IEC 61000-4-4	±2 kV for power supply lines ±1 kV for input/output lines	N/A	Mains power quality should be that of a typical commercial or hospital environment.
Surge IEC 61000-4-5	±1 kV differential mode ±2 kV common mode	N/A	Mains power quality should be that of a typical commercial or hospital environment.
Voltage dips, short interruptions, and voltage variations on power supply input lines IEC 61000-4-11	±5% U _T (>95% dip in U _T) for 0.5 cycle ±40% U _T (60% dip in U _T) for 5 cycles ±70% U _T (30% dip in U _T) for 25 cycles <5% U _T (>95% dip in U _T) for 5 sec.	N/A	Mains power quality should be that of a typical commercial or hospital environment.
Power Frequency (50/60 Hz) Magnetic Field IEC 61000-4-8	3 A/m	3 A/m	Power frequency magnetic fields should be at levels characteristic of a typical location in a typical commercial or hospital environment.
NOTE: U _T is the AC mains voltage before application of the test level.			

Table 3: Guidance and Manufacturer’s Declaration—Electromagnetic Immunity

Immunity Test	IEC 60601 Test Level	Compliance Level	Electromagnetic Environment—Guidance
<i>This device is intended for use in the electromagnetic environment specified below. The customer and/or user of this device should ensure that it is used in such an environment.</i>			
Portable and mobile RF communications equipment should be used no closer to any part of the device, including cables, than the recommended separation distance calculated from the equation applicable to the frequency of the transmitter.			
Conducted RF IEC 61000-4-6 Radiated RF IEC 61000-4-3	3 Vrms 150 kHz to 80 MHz 3 V/m 80 MHz to 2.5 GHz	3 Vrms 3 V/m	Recommended Separation Distance $d = 1.17 \sqrt{P}$ $d = 1.17 \sqrt{P}$ 80 MHz to 800 MHz $d = 2.33 \sqrt{P}$ 800 MHz to 2.5 GHz where P is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer and d is the recommended separation distance in meters (m). Field strengths from fixed RF transmitters, as determined by an electromagnetic site survey ^a , should be less than the compliance level in each frequency range ^b . Interference may occur in the vicinity of equipment marked with the following symbol: 

- a. Field strengths from fixed transmitters, such as base stations for radio (cellular/cordless) telephones and land mobile radios, amateur radio, AM and FM radio broadcast and TV broadcast cannot be predicted theoretically with accuracy. To assess the electromagnetic environment due to fixed RF transmitters, an electromagnetic site survey should be considered. If the measured field strength in the location in which the device is used exceeds the applicable RF compliance level above, the device should be observed to verify normal operation. If abnormal performance is observed, additional measures may be necessary, such as reorienting or relocating the device
- b. Over the frequency range 150 kHz to 80 MHz, field strengths should be less than [3] V/m.

NOTES:

- At 80 MHz and 800 MHz, the higher frequency range applies.
- These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects, and people.

Table 4: Recommended Separation Distances

The following table details the recommended separation distances between portable and mobile RF communications equipment and NR recorder.


<i>This device is intended for use in an electromagnetic environment in which radiated RF disturbances are controlled. Users of this device can help prevent electromagnetic interference by maintaining a minimum distance between portable and mobile RF communication equipment (transmitters) and the device as recommended below, according to maximum output power of the communications equipment.</i>			
Rated Maximum Output Power of Transmitter	Separation Distance According to Frequency of Transmitter(m)		
	150 kHz to 80 MHz $d = 1.17 \sqrt{P}$	80 MHz to 800 MHz $d = 1.17 \sqrt{P}$	800 MHz to 2.5 GHz $d = 2.33 \sqrt{P}$
W			
0.01	0.12	0.12	0.23
0.1	0.37	0.37	0.74
1	1.2	1.2	2.3
10	3.7	3.7	7.4
100	12	12	23

For transmitters rated at a maximum output power not listed above, the recommended separation distance d in meters (m) can be estimated using the equation applicable to the frequency of the transmitter, where P is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer.

NOTES:

- At 80 MHz and 800 MHz, the higher frequency range applies.
- These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects, and people.

FCC information

	<p>For patients with a pacemaker, maintain a minimum of 6 inches (15 cm) between the recorder and pacemaker. Turn the recorder off immediately and provide appropriate patient care if you suspect the recorder affected the pacemaker. The Health Industry Manufacturers Association recommends a minimum 6-inch (15 cm) distance between a wireless radio and a pacemaker, which is consistent with the recommendations of Wireless Technology Research.</p>
WARNING	

The NR device contains FCC ID: QOQBT121

This device complies with Part 15 of the FCC Rules. Operation is subject to the following conditions:

- This device may not cause harmful interference.
- This device must accept any interference received, including interference that may cause undesired operation.

This equipment has been tested and found to comply with the limits pursuant to Part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference in a residential installation. This equipment generates, uses and radiates radio frequency energy and, if not installed and used in accordance with the instructions, may cause harmful interference to radio communication. However, there is no guarantee that interference will not occur in a particular installation. If this equipment does cause harmful interference to radio or television reception, which can be determined by turning the equipment off and on, the user is encouraged to try to correct the interference by one or more of the following measures:

- Reorient or relocate the receiving antenna.
- Increase the separation between the equipment and receiver.
- Connect the equipment into an outlet on a circuit different from that to which the receiver is connected.
- Consult the dealer or an experienced radio/TV technician for help.

Document History

Version	Date	Updates	Changed by
1.0	01/01/2016	Initial document	Boris
2.0	18/06/2017	New Logo	Alex
2.1	06/07/2017	Add models to recorder feature matrix table; NR-1207-E and NR-314-T	Boris
2.2	24.09.2017	NR-1207-3 recording modes added	Alex
2.3	30.04.2018	Text corrections	Alex
2.4	11.12.2018	Accessory items list updated	Alex
2.5	12.11.2019	More languages support noted	Alex
2.6	25.11.2019	Norav GmbH new address	Alex
2.7	10.11.2020	General Updates	Michal, Boris
2.8	31.05.2021	Add description for RCM symbol on the label	Boris
2.9	31.08.2022	Add Part Number to the table in page 30	Michal Yeger